

# CM1950

## Cryostat

Supplemental Sheet to the Instructions for Use CM1950 1v8 Rev. I  
English

### Revision C

Always keep this document with the instrument.  
Read carefully before working with the instrument.

CE





## 1. Supplemental sheet to Instructions for Use CM1950 1v8 Rev. I

### Additional description to Chapter 12.3 Replacing the UVC lamp



#### Note

For the CM1950, two different variants of the connection piece inside the instrument and the UVC-Lamp are available. The user needs to check which variant is built-in in the instrument prior to the exchange of the UVC-Lamp with a new one.

The procedure to exchange the UVC-Lamp is similar with both variants.

#### Identifying the built-in variant and matching UVC lamp

- ① Variant 1: Connection piece with 2-pin inlet (→ Fig. 1-1), UVC lamp 2-pin (→ Fig. 1-2)

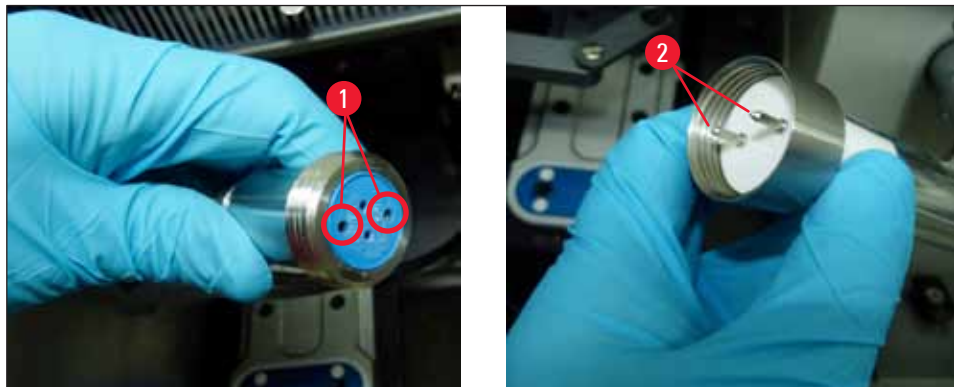


Fig. 1

- ① Variant 2: Connection piece with 4-pin inlet (→ Fig. 2-1), UVC lamp 4-pin (→ Fig. 2-2)

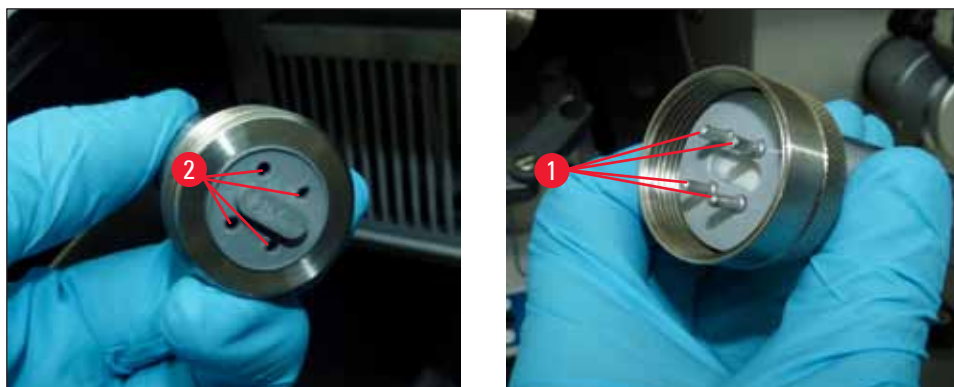


Fig. 2

Additional information to Chapter 12.3 Replacing the UVC lamp

New Fig. 95



Fig. 3

UV fluorescent tube - 2-pin

Order No. 14 0477 43192

New Fig. 96

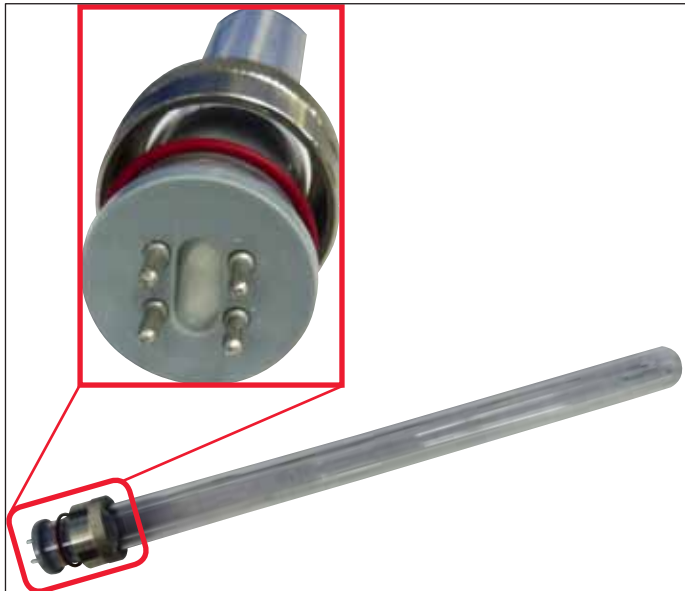


Fig. 4

UV fluorescent tube - 4-pin

Order No. 14 0471 57385



[www.LeicaBiosystems.com](http://www.LeicaBiosystems.com)



Leica Biosystems Nussloch GmbH  
Heidelberger Str. 17 - 19  
D-69226 Nussloch  
Germany

Tel.: +49 - (0) 6224 - 143 0  
Fax: +49 - (0) 6224 - 143 268  
Web: [www.LeicaBiosystems.com](http://www.LeicaBiosystems.com)