

Kreatech™ FISH probes

Product Information Sheet

KI-30505


Rab9b (XqF1) / WC Y Mouse probe

100 µl

DANGER



FORMAMIDE




Kreatech Biotechnology B.V.
Vlierweg 20
1032 LG Amsterdam
The Netherlands
www.LeicaBiosystems.com

RUO - Research Use Only

Not for use in diagnostic procedures

PI-KI-30505_D2.1

Published Sept 2015

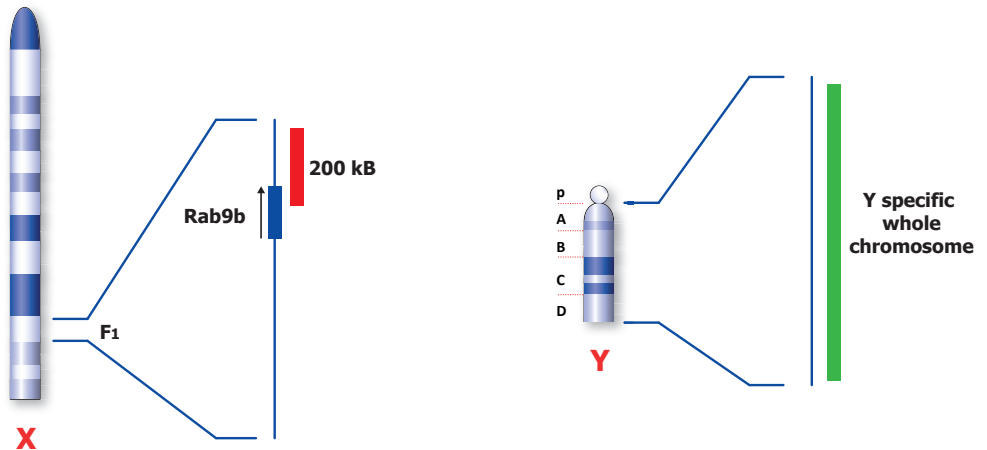

Not to scale

KI-30505

Kreatech™ Rab9b (XqF1) / WC Y Mouse FISH probe

- Introduction:** The **Rab9b (XqF1) / WC Y** mouse specific FISH probe is optimized to detect mouse chromosomes Y and X in a dual-color assay suited for mouse metaphase/interphase spreads, mouse blood smears and mouse bone marrow cells.
- Critical region 1 (red):** The **Rab9b (XqF1)** specific mouse FISH probe is direct-labeled with PlatinumBright™550.
Critical region 2 (green): The **WC Y** specific mouse FISH probe is direct-labeled with PlatinumBright™495.
- Reagent:** Kreatech probes are direct-labeled DNA probes provided in a ready-to-use format. Apply 10 µl of probe to a sample area of approximately 22 x 22 mm.
- Please refer to the Instructions for Use for the entire Kreatech FISH protocol.**
- Kreatech FISH probes are REPEAT-FREE™ and therefore do not contain Cot-1 DNA. Hybridization efficiency is increased and background, due to unspecific binding, is highly reduced.**
- Patterns:** The **Rab9b (XqF1) / WC Y** mouse FISH probe is designed as a dual-color assay to detect the mouse chromosomes Y and X. One single color red (R) and, one single color green (G) will identify the normal mouse chromosomes X and Y in a male, while two red signals will identify the normal mouse chromosomes X in a female. The signal for Chromosome Y appears as a colored area (like a paint) in interphase nuclei.
- Signal patterns other than those described above may indicate amplifications, deletions of mouse chromosome X and/or Y or other complex rearrangements.
- References:** Barchi et al, 2005, Mol Cell Biol, 25, 7203-7215
Bishop et al, 1987, Nucleic Acids Res, 15, 2959-2969
- Warning and precautions:** In case of emergencies check SDS sheets for medical advice. SDS sheets may be obtained by either contacting Leica Technical Support or visiting www.LeicaBiosystems.com. DNA probes contain formamide which is a teratogen; do not inhale or allow skin contact. Wear gloves and a lab coat when handling DNA probes. All materials should be disposed of according to your institution's guidelines for hospital waste disposal.
- Reagent Storage and Handling:** Store at 2-8 °C. Reagents should not be used after the expiration date on the vial label.
- TECHNICAL SUPPORT** Technical support is available at www.LeicaBiosystems.com/service-support/technical-support/ or toll free at 800-248-0123 or via e-mail: kreatech-support@leicabiosystems.com.
- CUSTOMER SERVICE** Kreatech probes may be ordered through Leica Customer Service toll free at 800-248-0123 or order via e-mail: purchase.orders@leica-microsystems.com.